

(Diagnostic Reagent Grade)

T-107

L- α -GLYCEROPHOSPHATE OXIDASE [GPOM]

from *Streptococcus* sp.

(sn-Glycerol-3-phosphate: oxygen 2-oxidoreductase, EC 1.1.3.21)



Preparation and Specification

Appearance : Yellowish amorphous powder, lyophilized

Specific activity : More than 15.0 U/mg solid

Properties

Substrate specificity	: See Table 1	
Molecular weight	: 169 kDa (TSK gel G 3000 SWXL gel filtration) 65 kDa (SDS-PAGE)	
Isoelectric point	: pH 4.4	
Michaelis constants	: L- α -Glycerophosphate 0.64 mM (pH 7.5)	
Optimum pH	: 8.5-9.0	Figure 1
pH stability	: 6.0-8.0 (37°C, 30 min)	Figure 2
Optimum temperature	: 37-42°C (pH 6.5)	Figure 3
Thermal stability	: Stable at 40°C and below (pH 6.5)	Figure 4
Effect of metal ions	: See Table 2	
Effect of detergents	: See Table 3	
Stabilizers	: FAD	

Applications for Diagnostic Test

This enzyme is useful for enzymatic determination of **triglyceride**.

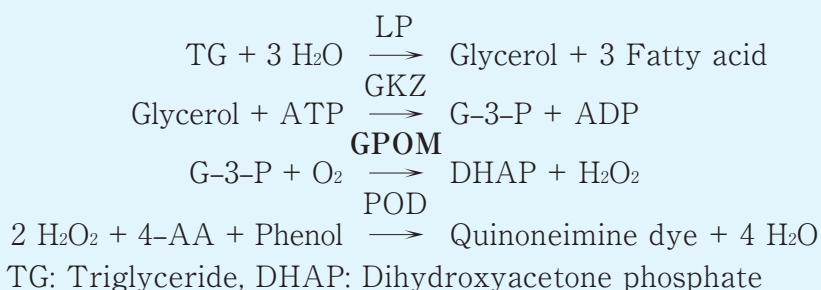



Table 1. Substrate specificity

Substrate (300mM)	Relative activity (%)
L- α -Glycerophosphate	100
Glucose-1-phosphate	0
Glucose-6-phosphate	0
Glycerol	0
Glucose	0

Table 3. Effect of detergents on GPOM activity


Detergent (0.1%)	Relative activity (%)
None	100
EMULGEN 810	98
EMULGEN 911	98
RHEODOL TWL-106	99
RHEODOL 460	99
ADEKANOL NP-720	99
Triton X-100	98
Triton X-305	99
Tween 80	98

Fig.1 Optimum pH

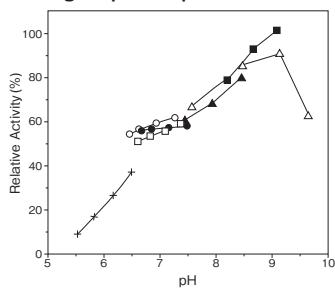

- 200 mM buffer
- : MES buffer
- : PIPES buffer
- : Phosphate buffer
- : Tris buffer
- △ : DEA buffer
- ▲ : TEA buffer
- + : Citrate buffer

Fig.2 pH Stability

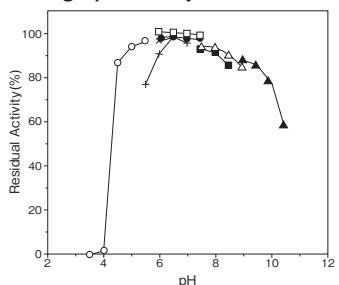


- 37°C, 30 min.
- 200 mM buffer
- : Citrate buffer
- : PIPES buffer
- : Phosphate buffer
- : Tris buffer
- △ : DEA buffer
- ▲ : Glycine buffer
- + : MES buffer
- × : Bis-Tris buffer

Table 2. Effect of metal ion on GPOM activity


Metal ion (2mM)	Relative activity (%)
None	100
MgCl ₂	101
MgSO ₄	102
ZnCl ₂	102
ZnSO ₄	102
NaCl	103
NH ₄ Cl	103
BaCl ₂	103
Ba(CH ₃ COO) ₂	101
NiCl ₂	103
CoCl ₂	103
MnCl ₂	114
LiCl	103
KCl	102
CaCl ₂	103

Fig.3 Optimum Temperature

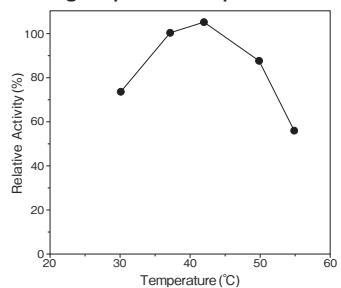

pH 6.5
200 mM PIPES buffer

Fig.4 Thermal Stability

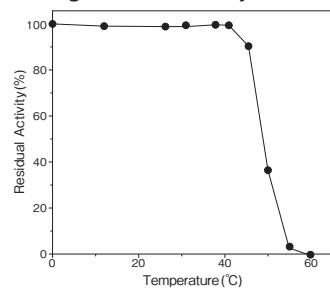


pH 6.5, 10min.
50 mM PIPES buffer

Assay

■ Principle

The assay is based on the increase in absorbance at 600 nm as the formation of quinoneimine dye in the following reactions:

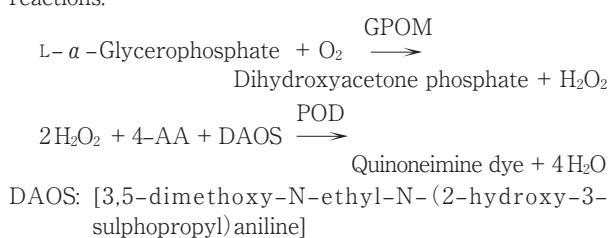

■ Unit definition

One unit is defined as the amount of enzyme which generates 1 μ mole of H_2O_2 per minute at 37°C under the conditions specified in the assay procedure.

■ Reagents

1. Reaction mixture

Dissolve 6.05 g of PIPES and 9.45 g (purity calculation) of Disodium Glycerophosphate with 70 ml of distilled water and adjust pH to 6.5 with 4 N NaOH at 25°C. Add all reagents listed below and confirm pH is 6.5 at 25°C. Add distilled water to make a total of 100 ml.

100 U/ml POD¹⁾ solution
15 mM 4-AA solution

100mM DAOS solution	1.0 ml
5% (W/V) Triton X-100 solution	1.0 ml
1):100 U/ml POD solution Dissolve 1,000 U (PPU) of POD with 10 ml of distilled water.	
2. Reaction stopper 0.5% (W/V) SDS solution SDS: Sodium dodecyl sulfate	
3. Enzyme dilution buffer 10 mM PIPES-NaOH buffer pH 6.5 containing 0.1% (W/V) Triton X-100	
4. Reagents PIPES [Piperazine-1,4,-bis (2-ethanesulfonic acid)]: Dojindo Laboratories # 345-02225 DAOS (sodium salt) : Dojindo Laboratories #OC06 4-AA: NACALAI TESQUE, INC. Special grade #01907-52 Triton X-100: The Dow Chemical Company Disodium Glycerophosphate 5.5 Hydrate : FUJIFILM Wako Pure Chemical Corporation #192-02055 SDS (Sodium Dodecyl Sulfate) : NACALAI TESQUE, INC. Extra pure #31606-75 POD: Sigma Chemical Co. Type II #P-8250	

■ Enzyme solution

Accurately weigh about 20 mg of the sample and add enzyme dilution buffer to make a total of 20 ml. Dilute it with enzyme dilution buffer to adjust the concentration as required.

■ Procedure

- Pipette accurately 1.0 ml of reaction mixture into a small test tube and preincubate at 37°C.
- After 5 min, add exactly 20 μ l of enzyme solution and mix to start the reaction at 37°C.
※ In the case of a test blank, add 20 μ l of enzyme dilution buffer in place of enzyme solution.
- At 5 min after starting the reaction, add 2.0 ml of the

reaction stopper to stop the reaction.

4. Measure the absorbance at 600 nm.

Absorbance sample : As

blank : Ab

$$0.1 \text{ Abs} \leq \Delta A (\text{As} - \text{Ab}) \leq 0.2 \text{ Abs}$$

■ Calculation

$$\text{Activity (U/mg of powder)} = \frac{\Delta A / 5}{16.8 \times 1/2} \times \frac{3.02}{0.02} \times \frac{1}{X}$$

16.8 : millimolar extinction coefficient of quinoneimine dye at 600 nm ($\text{cm}^2 / \mu\text{mole}$)

1/2 : a multiplier derived from the fact that 2 mole of H_2O_2 produces 1 mole of quinoneimine dye

5 : reaction time (min)

3.02 : final volume (ml)

0.02 : volume of enzyme solution (ml)

X : concentration of the sample in enzyme solution (mg/ml)

Storage

Storage at -20°C in the presence of a desiccant is recommended. Enzyme activity will be retained for at least one year under this condition.

References

- Jacobs, N. J. and Van Demark, P. J. (1960) Arch. Biochem. Biophys., **88**, 250-255.
- Koditschek, L. K. and Umbreit, W. W. (1969) J. Bacteriol., **98**, 1063-1068.
- Gancedo, C., Gancedo, J. M. and Sols, A. (1968) J. Biochem. (Tokyo), **5**, 165-172.
- Kistler, W. S., Hirsch, C. A., Cozzarelli, N. R. and Lin, E. C. (1969) J. Bacteriol., **100**, 1133-1135.
- Esders, T. W. and Michrina, C. A. (1979) J. Biol. Chem., **254**, 2710-2715.

GPOM 活性測定法 (Japanese)

I. 試薬液

1. 反応試薬混合液

PIPES 6.05g とグリセロリン酸 2Na 9.45g (純度換算) を精製水 70ml に溶解した後、4N NaOH で pH6.5 (25°C) に調整し、その液に下記試薬を加えて混和し、pH6.5 (25°C) であることを確認した後、精製水で全容 100ml とする。

100U/ml POD 溶液 ¹⁾	5.0 ml
15mM 4-AA 溶液	10.0 ml
100mM DAOS 溶液	1.0 ml
5% (W/V) トリトン X-100 溶液	1.0 ml

1):100U/ml POD 溶液

POD 1,000 単位 (PPU) を精製水 10ml で溶解する。

2. 反応停止液

0.5% (W/V) SDS 溶液

3. 酵素溶解希釈用液

0.1% (W/V) トリトン X-100 を含む 10mM PIPES-NaOH 緩衝液 pH6.5

4. 試薬

PIPES [ピペラジン-1,4-ビス(2-エタノールホン酸)] : 同仁化学製 #345-02225

DAOS [3,5-ジメトキシ-N-エチル-N-(2-ヒドロキシ-3-スルホプロピル)アニリン] : 同仁化学製 #OC06

4-AA : ナカライテスク製 特級 #01907-52

トリトン X-100 : Dow Chemical 製

グリセロリン酸二ナトリウム 5.5 水和物 :

富士フイルム和光純薬製 #192-02055

SDS (デシル硫酸ナトリウム) :

ナカライテスク製 一級 #31606-75

POD : シグマ製 Type II #P-8250

II. 酵素試料液

検品約 20mg を精密に量り、酵素溶解希釈用液で溶解して全容 20ml とする。

その液を酵素溶解希釈用液で適宜希釈する。

III. 測定操作法

1. 小試験管に反応試薬混合液 1.0ml を正確に分注し、37℃で予備加温する。
2. 5 分経過後、酵素試料液 20 μ l を正確に加えて混和し、37℃で反応を開始する。
- ※盲検は酵素試料液の代わりに酵素溶解希釈用液 20 μ l を加える。
3. 5 分経過後、反応停止液 2.0ml を加えて混和し、反応を停止する。
4. 600nm における吸光度を測定する。

求められた吸光度を試料液は As、盲検液は Ab とする。

$$0.1 \text{ Abs} \leq \Delta A = (As - Ab) \leq 0.2 \text{ Abs}$$

IV. 計算

$$\text{活性 (U/mg)} = \frac{\Delta A/5}{16.8 \times 1/2} \times \frac{3.02}{0.02} \times \frac{1}{X}$$

16.8 : キノンイミン色素の 600nm におけるミリモル分子
吸光係数 ($\text{cm}^2/\mu\text{mole}$)

1/2 : H_2O_2 2 モルからキノン色素 1 モルが生成することによる係数

5 : 反応時間 (min)

3.02 : 反応に供した酵素試料液量 (ml)

X : 酵素試料液中の検品濃度 (mg/ml)